Biomedical Optics EXPRESS

Multiplexed COVID-19 antibody quantification from human sera using label-free nanoplasmonic biosensors: supplement

WIHAN ADI, 1 DHRUV BISWAS, 1 MIRIAM A. SHELEF, 2,3 AND FILIZ YESILKOY 1,* D

This supplement published with Optica Publishing Group on 16 March 2022 by The Authors under the terms of the Creative Commons Attribution 4.0 License in the format provided by the authors and unedited. Further distribution of this work must maintain attribution to the author(s) and the published article's title, journal citation, and DOI.

Supplement DOI: https://doi.org/10.6084/m9.figshare.19317365


Parent Article DOI: https://doi.org/10.1364/BOE.454919

¹Department of Biomedical Engineering, University of Wisconsin-Madison, Madison, WI 53706, USA

²Department of Medicine, University of Wisconsin-Madison, Madison, WI 53705, USA

³William S. Middleton Memorial Veterans Hospital, Madison, WI 53705, USA

^{*}filiz.yesilkoy@wisc.edu

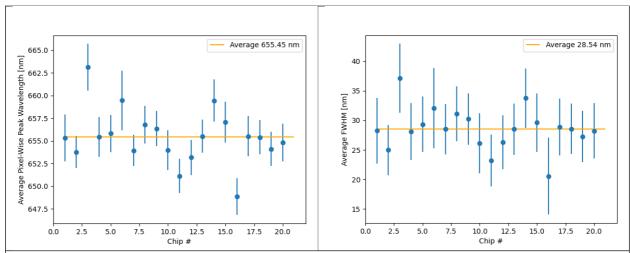

S1. Average wavelength of spectral peaks in each pixel for each of the 20 studied AuNHA chips (left) and their full-width half maximum (right)

